

Mai Tai™ Hybridization System USER MANUAL

Cat. #1075-00-1, 1075-00-2



FOR RESEARCH USE ONLY
Not for Use in Diagnostic Procedures

Serial Number

The following serial number identifies the specific instrument you have purchased and must be referenced when requesting service. A copy is affixed to the instrument.

Technical Service: (408) 733-7337, techserv@scigene.com

Warranty

SciGene warrants that the heating unit described in this manual shall be free of defects in materials and workmanship for a period of 12 months from date of delivery. This warranty does not cover removable blocks or accessories. In the event of a defect during the warranty period, SciGene's limit of liability will be to provide replacement parts at no charge or, at its sole discretion, replace the product. The foregoing warranty is void in the event the unit was abused or modified or used in a manner inconsistent with its intended purpose. SciGene makes no other warranty, expressed or implied including warranties of merchantability and fitness for a particular purpose. In no event shall SciGene be liable for any direct, indirect, special, incidental or consequential damages or for any damages resulting from loss arising out of or in connection with the sale, use or performance of the product.

Copyright

Copyright ©2008 SciGene Corporation. All rights reserved. SciGene is a trademark of SciGene Corporation, Sunnyvale, CA. All other trademarks used in this manual are the property of their respective owners.

Table of Contents

I. SAFETY NOTICES	3
A. Intended Use	3
B. Instrument Safety	3
C. Warnings	3
D. Cautions	3
E. Lifting and Moving the Unit.....	3
II. UNPACKING AND SETTING UP YOUR OVEN.....	4
A. Removing the Unit from the Carton.....	4
B. Parts Provided.....	4
C. Installation	4
III. USING YOUR OVEN.....	5
A. Oven Components and Controls	5
B. Closing and Opening the Door.....	6
C. Using the Temperature Controller.....	6
D. Setting Rotator Speed	6
E. Using the Jog Switch	6
F. Calibrating the Oven Temperature	7
G. Loading and Removing Rotators.....	8
IV. USING MAI TAI™ HYBRIDIZATION CASSETTES.....	9
V. CLEANING AND STORAGE OF MAI TAI™ HYBRIDIZATION CASSETTES ...	11
VI. MAINTAINING YOUR OVEN	12
A. Servicing.....	12
B. Cleaning.....	13
VII. TROUBLESHOOTING.....	14
VIII. SPECIFICATIONS.....	14
IX. CHAMBERS, ROTATORS AND ACCESSORIES.....	14

I. SAFETY NOTICES

A. Intended Use

This instrument is intended for the heating and incubation of laboratory samples. This instrument should only be used according to the instructions provided in this manual. If the equipment is used in a manner not specified by the manufacturer, the protection provided by the equipment may be impaired.

B. Instrument Safety

Before operating the instrument, read the information in this section concerning hazards and potential hazards. Ensure that anyone involved with the instrument's operation is instructed in both general safety practices for laboratories and specific safety practices for the instrument.

C. Warnings

Failure to comply with the following warnings that are affixed to the product can lead to possible personal injury or death.



D. Cautions

Failure to comply with the following cautionary statement affixed to the product may lead to possible personal injury. Items heated in the oven should be handled with heat protective gloves.

Open all closed vessels heated in the oven with the opening pointed away from you to avoid contact with heated aerosols.



E. Lifting and Moving the Unit

The rotating oven you have purchased weighs approximately 70 lbs (32 kg). Use caution when lifting the unit to protect you and others from personal injury. It is strongly recommended that two people lift the unit simultaneously to keep it balanced and to share the load.

II. UNPACKING AND SETTING UP YOUR OVEN

A. Removing the Unit from the Carton

Position the shipping carton on the floor close to the location of intended installation. Remove the foam inserts from the top of the unit. Position one person at the front and one at the back of the oven. Grip the recessed edges along the top of the unit and lift it straight up and out of the shipping carton taking care to keep it balanced. Place it on the bench or table where it will be installed.

Carefully inspect the unit for damage. If there is evidence of damage, do not discard the shipping materials since they may be needed to return the unit.

B. Parts Provided

The following items are included with the system.

- Model 777 Microarray Oven
- Mai Tai™ Rotator
- Mai Tai™ Cassettes (2x)
- Oven Power Cord
- User Manual

C. Installation

1. Placement

Place the unit on a stable, level surface within a few feet of the power source. Avoid locating it below a shelf where solutions are stored. A spill may enter the electrical compartment through the vent holes on the top of the unit and cause damage. Ensure there is adequate clearance along the front and right side of the oven to open the door completely.

There should be a minimum clearance of 3 inches along the top and back panels for air circulation.

2. Connecting the Power

Plug the power cord provided into the back of the unit and then to a properly grounded outlet. Use only the power cord provided.


3. Powering On

Turn power ON to the unit using the switch on the front of the unit.

III. USING YOUR OVEN

A. Oven Components and Controls

- **Power Switch** -Turns on main power to unit.
- **Temperature Controller** - Used to set and observe chamber temperature
- **Rotator Control** -Turns on and controls the speed of the rotator
- **Jog Switch** - Activates rotator with door open at the speed selected.
- **Door Latch** - Tightly secures the door closed with button release to open

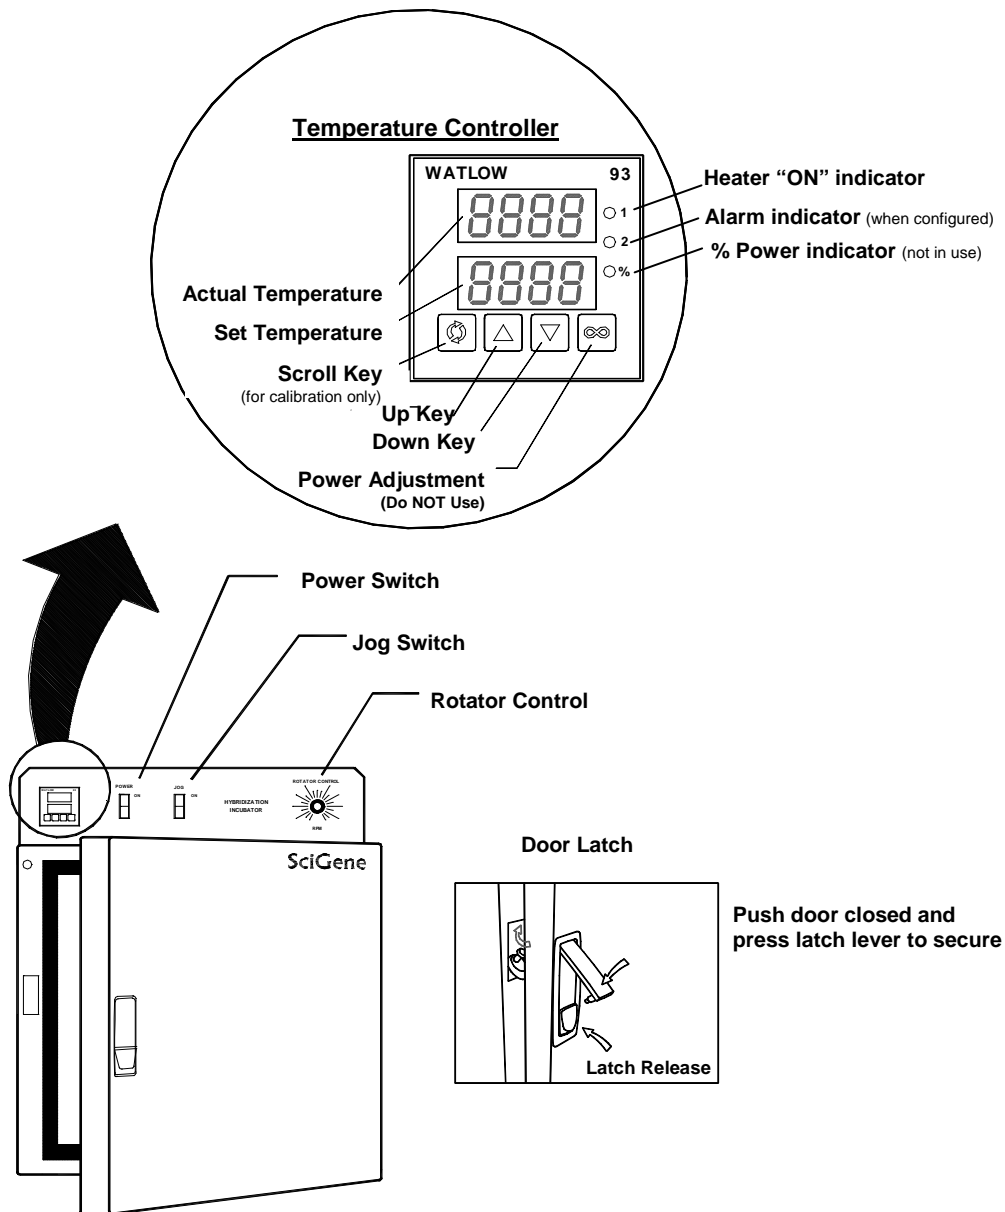

B. Closing and Opening the Door

To secure the door, press the door against the cabinet to close and push down the top lever. To open, press the lower latch release button.

C. Using the Temperature Controller

The features of the Watlow 93 temperature controller on your oven are shown in the illustration (Section III A). It has two LED readouts and four membrane buttons. The upper readout displays the ACTUAL temperature. The lower readout displays the SET chamber temperature. The button with the circle icon at the lower left is used to scroll through the controller parameters when performing calibration of the controller. It is *not* used during normal operation. The up and down arrow buttons are used to adjust the desired set temperature. They are also used when calibrating the oven.

The infinity symbol (∞) button on the lower right of the panel is for adjusting the power that is delivered to the chamber heaters. It is set at 100% at the factory and *should not* be adjusted during normal operation.

To set oven temperature, simply push the up and down arrows until the desired temperature is shown. The unit will now adjust the heat of the chamber until the SET temperature is attained.

The controller is calibrated at the factory to provide an accurate chamber temperature when operated from ambient + 5 to 99°C. It is recommended that the temperature controller be recalibrated monthly to ensure accurate oven temperatures.

D. Setting Rotator Speed

The rotator is turned on and off and its speed of rotation controlled through the rotary switch. Turn the dial clockwise from its stopping point to turn on the rotator drive system and set the speed of rotation. Rotation speed is adjustable from 2 to 80 RPM.

E. Using the Jog Switch

The jog switch is used to momentarily advance the rotator when the door is open. When the jog switch is pressed, the rotator will turn at the speed selected on the speed controller. It will not move if the speed controller is turned off or is set below 2 RPM.

F. Calibrating the Oven Temperature


The Watlow 93 temperature controller comes calibrated by SciGene to provide accurate chamber temperatures from ambient +5 to 99°C.

Calibration of the controller is required *only* if, when verifying with a NIST-certified digital thermometer (SciGene Cat. #1051-52-0), the chamber temperature differs by *more than one degree* from the actual temperature shown on the display.

Do not use a glass thermometer.

To adjust the controller to achieve accurate oven temperatures:


1. With the oven powered on, enter a temperature of 65°C on the controller and allow the temperature on the display to stabilize (about 20 minutes).
2. Using the cable provided with the digital thermometer, plug one end into the blue jack found on the back panel and the other into the digital thermometer. Turn ON the thermometer.
3. On the temperature controller, press the up and down arrows simultaneously for 3 seconds. The upper display will now read “3” and the lower display “Loc”.
4. Using the down arrow, set the upper display to “0” The controller is now unlocked and available for calibration.
5. Sequentially press the circle icon button until the display shows the **Actual** and **Set** temperatures of the oven.
6. Calculate the difference in temperature shown on the **Actual** display of the controller and the digital thermometer. For example, if the controller displays 52.5°C and the digital thermometer displays 51.0°C, the difference is 1.5°C.
7. Sequentially press the circle icon button until the lower display reads “Cal”. The upper display shows the offset value between the controller and digital thermometer when the unit was last calibrated.
8. Using the up and down arrows, adjust the offset value to the difference in temperatures calculated in Step 6. For example, if the controller displays a temperature that is 1.5°C higher than the digital thermometer, adjust the offset value to *minus* 1.5.

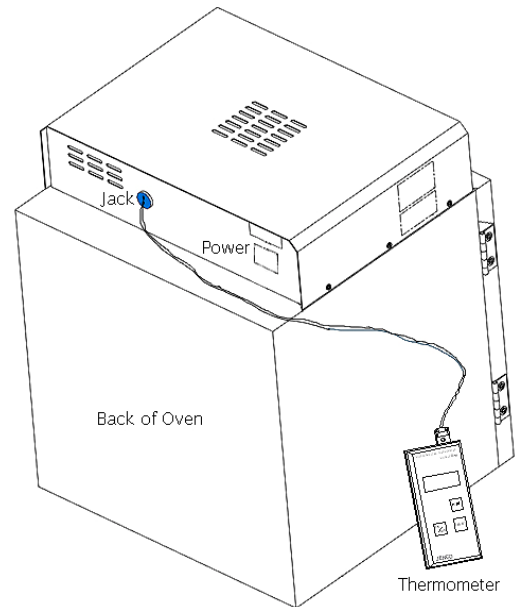


9. Sequentially press the circle icon button until the display shows the **Actual** and **Set** temperatures. The **Actual** temperature on the display should now match the digital thermometer.
10. Press the circle icon button until “**Loc**” is shown on the lower display. Press the up arrow until 3 is shown in the upper display.
11. Sequentially press the circle icon button until the **Actual** and **Set** temperatures are again shown on the display.

Your oven is now calibrated to provide accurate temperatures between ambient +5 to 99°C.

G. Loading and Removing Rotators

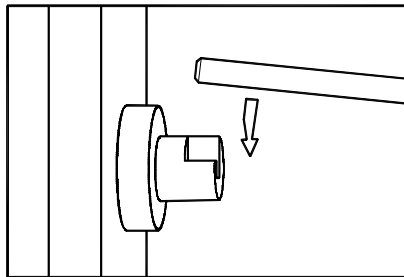

Place end of shaft on left bearing

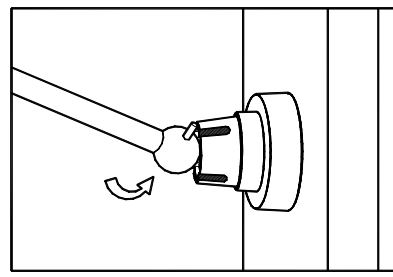

Insert shaft ball with alignment pin into right bearing

All rotators are loaded and removed using the same two-step process. When loading, first insert the end of the shaft that ends in a ball joint with alignment pin into the slotted bearing on the right wall of the chamber. The left end of the shaft is then placed into the bearing on the left side of the chamber. Reverse this procedure when removing the rotator.

IV. USING MAI TAI™ HYBRIDIZATION CASSETTES

1. With Mai Tai™ Rotator installed, pre-heat the hybridization oven to the desired incubation temperature.
2. Place the base plate on a flat surface such as a laboratory bench.
3. Place a gasket slide into each chamber in the cassette with the “Agilent” label facing up and aligned with the “barcode” side of the chamber, as shown in Figure 2.



When placing the gasket slide, make sure the slide does not rest on the edge of the base plate (Figure 3). To familiarize new users with the placement technique, practice placing ordinary 1” x 3” (25 mm x 75 mm) glass slides into the chamber prior to running an experiment.

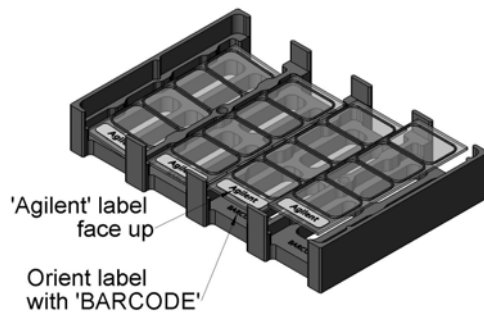


FIGURE 2

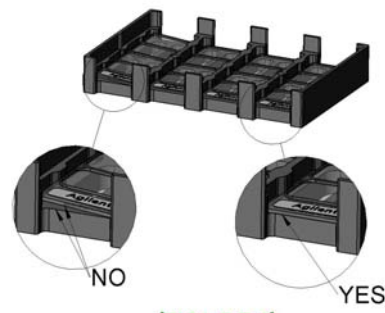


FIGURE 3

4. Pipette the labeled probe into each chamber of the gasket slide using the volumes shown in the table below for each gasket slide format.



To prevent spilling or leaking, dispense the hybridization solution to the center of the gasket well without touching the gasket with the pipette tip. Figure 4 shows hybridization solution added to a 4 x gasket slide.

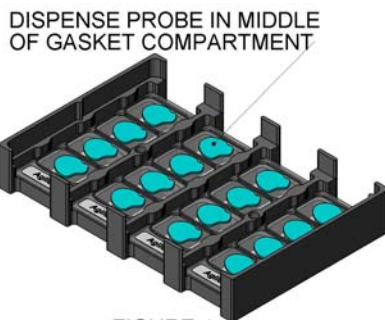


FIGURE 4

Gasket Format	Probe Volume
1x microarray	520 μ l
2x microarray	260 μ l
4x microarray	110 μ l

5. Holding array at the ends **with the array side down** and ensuring that the barcode side matches with the one on the gasket slide, bring the array down slowly holding it horizontal to the gasket slide (Figure 5).

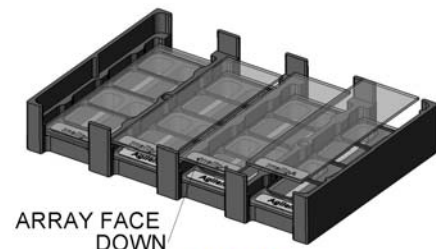




FIGURE 5

 Placing the array evenly onto the gasket slide is crucial to prevent spilling or leakage.

 Use Agilent arrays or microarrays from other sources that are compatible with the Agilent gasket slides.

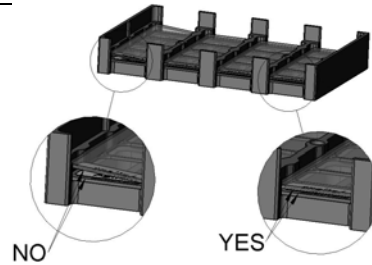


FIGURE 6

6. When all arrays have been placed, make sure all assemblies are laid flat against the base plate. See Figure 6 for examples of proper and improper placement.

7. Place the cover plate over the arrays with the barcode window matching the barcodes on array. See Figure 7 showing correct placement and orientation of the cover plate.

8. Tighten the thumb screws all the way to a complete stop. Do not use tools.

9. Rotate the cassette to ensure that the bubbles move freely inside each array chamber.

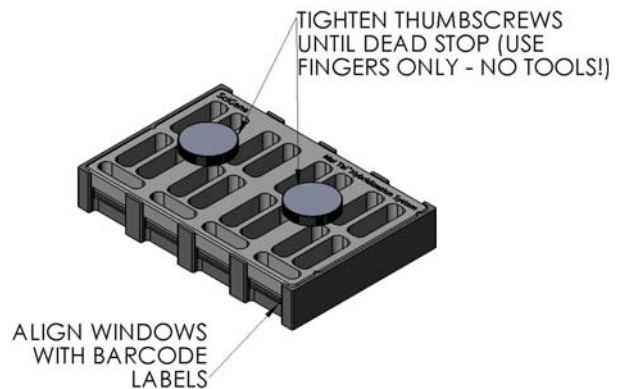




FIGURE 7

 For optimal hybridization, it is best to have a single, large bubble which moves freely around the chamber when rotated. After assembly, ensure that there are no stationary bubbles in any array chamber when the assembly is rotated. Stationary bubbles can be released by gently tapping each corner of the assembly on a firm surface as it is rotated.

10. Place the assembly into the Mai Tai™ Rotator in the pre-heated oven. Raise the spring bar and load each Mai Tai™ Cassette into the sleeves of Mai Tai™ Rotator as shown in Figure 8.

 When loading multiple cassettes, load equal number of cassettes on either sides of the rotator to balance weight.

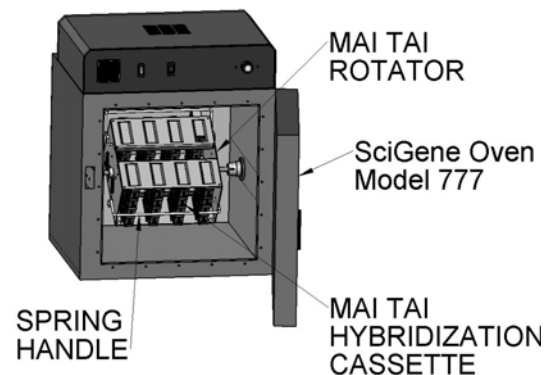


FIGURE 8

11. Rotate the Mai Tai™ Rotator at the speed and time recommended by the microarray manufacturer.

12. At the completion of the incubation period, remove the cassette(s) from the rotator and allow to cool for a few minutes. Loosen thumbscrews and remove the top plate.

13. One-at-a-time, remove the array gasket slide “sandwich” and separate them while submerged in the buffer specified by the array supplier.

14. Wash and dry the microarray on the Little Dipper Processor [SciGene Cat. #1080-40-1 (115v); 1080-40-2 (220v)] or manually using the buffer specified by the array supplier.

V. CLEANING AND STORAGE OF MAI TAI™ HYBRIDIZATION CASSETTES

Hybridization solution may occasionally spill and dry on to Mai Tai™ base and cover plates, making arrays or gasket slides stick to these parts during hybridization. Base plates, cover plates and thumb screws need to be cleaned periodically to prevent such sticking. Follow the protocol below to clean Mai Tai™ parts.

1. Disassemble each Mai Tai™ cassette into base plate, cover plate and thumb screws. Captive thumb screws can be unscrewed from the cover plate.
2. Using a lint-free wipes soaked in 70% ethanol, wipe all surfaces of base plate, cover plate, thumb screws and thumb screw hole carefully to remove dried hybridization solution and salts.
3. Allow the clean parts to dry completely by evaporation.
4. Assemble the parts back together using the thumb screws and store in a dry place.

VI. MAINTAINING YOUR OVEN

A. Servicing


Turn the power switch to the OFF position and unplug the power cord before performing any service procedure.

1. Checking and Replacing Fuses

Fuses are located in a removable fuse block below the power cord receptacle on the back of the unit.

Unplug the cord and using a flat blade screwdriver, remove the fuse block as shown in the illustration. Remove the fuse holder from the block and gently remove the two fuses. A blown fuse will appear dark.

Always replace a blown fuse with fuses matching the amperage and voltage as shown on the label below the fuse block.

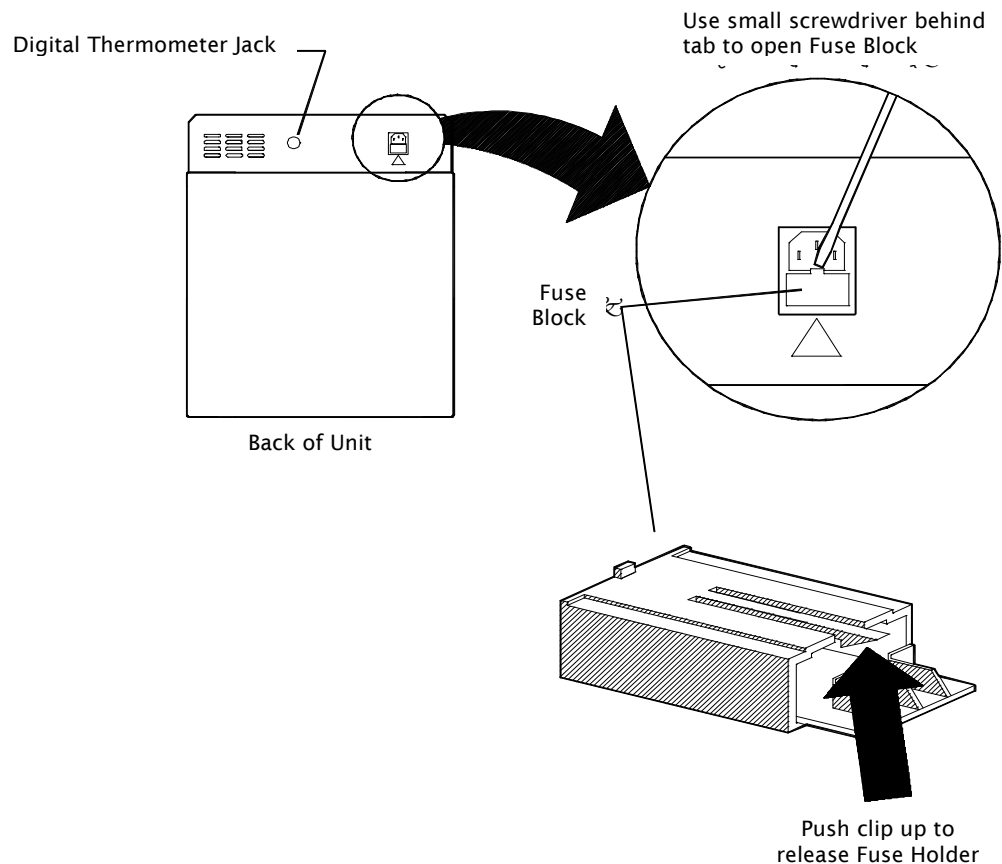

2. Replacing the Temperature Controller

If the actual temperature reported on the controller is erratic after calibration, the temperature controller may need to be replaced. Please contact SciGene Technical Services (techserv@scigene.com) for assistance in troubleshooting. If needed, replacement controllers are available (SciGene cat. #RP600-0146-03).

3. Rotator Drive System

The rotator drive system is designed to provide trouble-free operation for many years and does not require routine maintenance. However, components of the drive system that fail due to normal wear and tear over long-term usage can be easily replaced. Contact SciGene's Technical Service Department (techserv@scigene.com) to obtain replacement parts and perform these repairs.

B. Cleaning

Clean the exterior and interior surfaces using a mild, detergent-based spray cleaner and wipe with a soft cloth.

Under no circumstances should solutions be allowed to enter the electronics package through the ventilation slots on the top of the unit.

Do not use abrasive cleansers or scouring pads that can scratch the stainless steel.

VII. TROUBLESHOOTING

Symptom	Cause	Solution
Rotator does not turn after closing door	Rotator control is in the off position	Turn on rotator
Door does not shut or is difficult to open	Latch is improperly adjusted	Adjust threaded rod on inside of latch
Temperature is erratic	Thermal controller is defective	Replace controller

VIII. SPECIFICATIONS

Electrical (Model 777 Oven)	
Cat. #1077-00-1	115/120V AC; 50/60 Hz; 350 W
Cat. #1077-00-2	220/240V AC; 50/60 Hz; 350 W
Dimensions	
Interior Chamber	14 W x 14 D x 14 H inches
	36 W x 36 D x 36 H cm
Exterior	18 W x 17 D x 22 H inches
	45 W x 40 D x 56 H cm
Weight	
Net	70 lbs (32kg)
Gross	75 lbs (34kg) Includes shipping carton
Performance and Controls	
Temperature Range	Ambient + 5°C to 99°C
Temperature Control	± 0.1°C
Heat up Time	3°C per minute
Temperature Controller	Digital PID, single loop
Temperature Display	Actual / Set Dual LED
Rotation Speed	2 to 80 RPM
Chamber	Stainless Steel
Digital Thermometer Output	Thermocouple

IX. CHAMBERS, ROTATORS AND ACCESSORIES

Cat. #	Description	UOM
1075-10-0	Mai Tai Hybridization Cassette. Holds four slides.	Each
1051-52-0	Handheld electronic digital thermometer with Type T thermocoupler—includes NIST traceable certificate of calibration and interface cable.	Each
1077-30-0	Rotator for 96 Affymetrix GeneChips.	Each
1077-10-0	Rotator for 48 Affymetrix GeneChips.	Each
1070-20-0	Rotator for 20 Agilent SureHyb and Original Version Hybridization Chambers.	Each
1052-23-0	General Purpose Rotator	Each
1052-24-0	Loading Stand for General Purpose Rotator	Each
1040-21-0	Removable Rocking Platform	Each
1040-21-1	Standard 10/20 tube rotator for Series 700 Ovens	Each
1040-01-0	Hybridization tube, 35 x 300 mm with screw cap	Each
1040-02-0	Hybridization tube, 35 x 150 mm with screw cap	Each